


5973 Air and Water Check

Instrument: MSD22

Sun Jul 23 10:12:58 2006

C:\MSDCHEM\1\5973N\

Scan: 10.00 - 75.00 Samples: 8 Thresh: 0 Step: 0.10  
 69 peaks Base: 69.00 Abundance: 322304

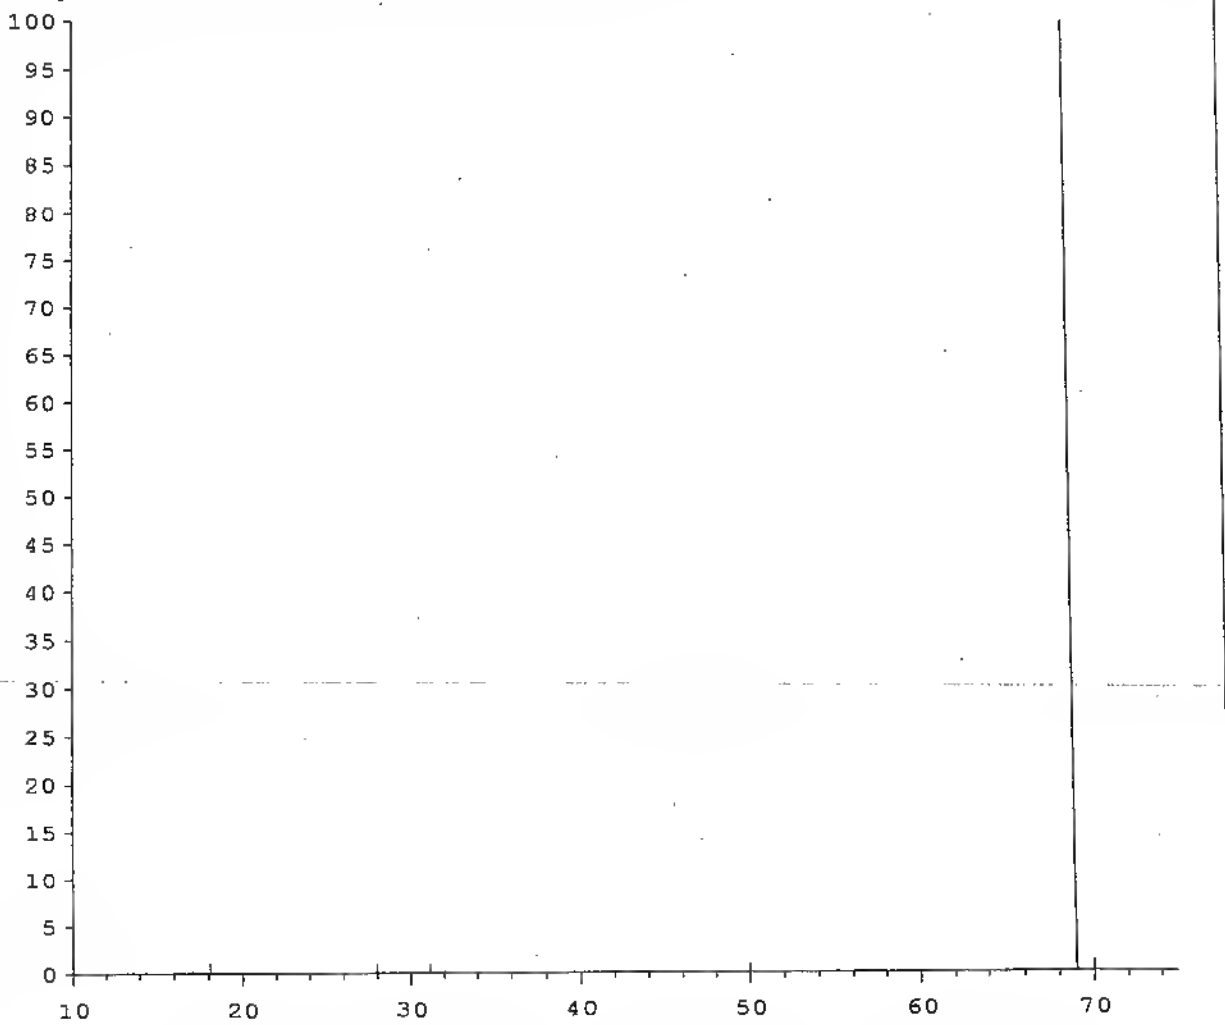

Mass	Abund	Rel Abund	Iso	Mass	Iso Abund	Iso Ratio
69.00	322304	100.00		70.00	3612	1.12
18.10	3336	1.04		19.00	34	1.02
28.00	3013	0.93		28.90	58	1.92

Current Params used: ATUNE.U

Relative abundances:

18/69 = 1.04	Water%
28/69 = 0.93	Nitrogen%
32/69 = 0.28	Oxygen%
44/69 = 0.17	Carbon Dioxide%
28/18 = 90.32	Nitrogen/Water%